



# ARM Processor Based Wireless Data Acquisition System for Pressure Distribution Analysis

Ms. Pavithra M<sup>1</sup>, Ms. Jayanthi K<sup>2</sup>, Ms.Kanimozhi R<sup>3</sup>, Ms.Priya N<sup>4</sup> and Mr.Ramesh.K<sup>5</sup>

<sup>1,2,3,4</sup>UG students Department of Electronics and Communication Engineering, V.R.S.College of Engg & Tech, Villupuram, Tamil Nadu, India

<sup>5</sup>Assistant Professor, Department of Electronics and Communication Engineering, V.R.S.College of Engg & Tech, Villupuram, Tamil Nadu, India

**Abstract:** Techniques that could precisely monitor human motion are useful in applications such as rehabilitation, virtual reality, sports science, and surveillance. Pressure distributions in the human feet are important and useful measures in footwear evaluation, athletic training, clinical gait analysis, and pathology foot diagnosis. Most of the existing systems require wiring that restrains the natural movement and are also uncomfortable to wear. Commercially available systems are too expensive for small establishments. To overcome these limitations, a wearable wireless sensor network using low-cost, low-power wireless sensor platform implemented using an IEEE 802.15.4 wireless standard can be developed with compact wearable sensors. An embedded system using ARM processor has been considered for the hardware and to gain access to laptop, which can be configured to comfortably work in research laboratories, clinics, sport ground, and other outdoor environments. A method by which an interactive front end can be developed for this application has been discussed. The results are displayed as values by instantaneous signals and pie charts. Also provision has been made to calculate and display peak pressure and mean pressure at a given point.

**Keywords:** Foot pressure measurement, wireless sensor network, biomedical application, embedded system, ARM processor.

## I. INTRODUCTION

Measurement of footpressure that is present in the human foot is called plantar pressure measurement which is an useful parameter which can be effectively used in various commercial and medical applications. At the first instant it can has the commercial application of evaluation of footwear. It can be used to evaluate the effectiveness of therapeutic and athletic shoes with and without visco elastic insoles, using the mean peak plantar pressure as the parameter. Secondly it can be used in application related to athletic training for optimizing sports performance with thin-film pressure sensors and relatively inexpensive data acquisition hardware. More researches have been reported on athletic plantar pressure analysis in order to improve sports achievements, such as soccer balance training and forefoot loading during running.

Clinical gait analysis, the investigation of the pattern of walking, is the third application. Plantar pressure distribution was employed to detect gait patterns: normal gait, toe in, toe out, over supination, and heel walking gait abnormalities. Plantar pressure was applied in pathology like assessment of the diabetic foot. A variety of plantar pressure measurement systems are available in the market or in the research laboratories. With respect to their technical specifications and intended application, in general, there are two main types of devices: platform systems and in-shoe systems. Platform systems are usually embedded in a walkway. However,

this kind of system is restricted to use in a laboratory or hospital, and used for barefoot measurements. In-shoe systems can be used to record the plantar pressure distributions within a shoe. Commercial products available from companies like Tekscan, Inc., capture dynamic in-shoe temporal and spatial pressure distributions, which were utilized for dynamic gait stability analysis, gait detection, and altered gait characteristics during running. However, those systems use electrical wires to connect in-shoe sensors and data acquisition system around the waist, which cause inconvenience and discomfort during strenuous exercises. A wireless structure shoe-integrated sensor system was developed for gait analysis and real-time feedback. In the system, hard devices have been used as the sensing units, which are not comfortable and cannot last for a long time because of fatigue of the sensing units. The data acquisition systems are often large and cannot be configured to connect with different remote receivers.

## II. HARDWARE

### A. Design Objectives

With the purpose of collecting valid accurate data in natural condition of activities, the plantar pressure measurement system should have the following features. First, it should be wearable without intervening with the regular activity of the wearer. Secondly the sensing unit



has to perform with consistency for repeated testing. Thirdly the system should be convenient to wear. Usage of wireless technology to transfer data would be the most convenient system to be established. Taking into consideration the above requirements here we present a pressure measurement and analysis technique employing wireless transmission. Design of a data acquisition system and stable sensor network has been discussed. A software for setting the hardware parameter and to monitor pressure values has been discussed.

**B. Sensor Selection**

Based on the aforementioned requirements, this paper presents an in-shoe plant pressure measurement and analysis system based on a fabric pressure sensing array. A textile pressure sensing array whose internal structure has been shown in fig 1(a) has been considered.

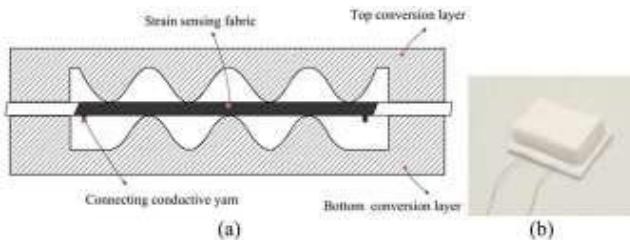


Fig. 1. Textile pressure sensor. (a) Schematic diagram of the structure of the pressure sensor (side view). (b) Package outlook.

It has a strain gauge factor of approximately 10 or above and excellent fatigue resistance (>100 000 cycles) for strain up to 40%. The sensor measurement ranges are from 10 Pa to 800 kPa, suitable for a wide variety of human-apparel interfaces, such as loosely fit garment walking/running shoes etc. The sensor is packaged by silicon rubber so that moisture and dust will not affect its performance, as shown in Fig. 1(b).

Several textile pressure sensors are connected in an  $n + 1$  line structure to construct a sensor array. One line is connected to each sensor as the  $-1$  ground line of the sensor array. Another line of each sensor is the output as the  $-n$ th signal line for the sensor array that contains  $n$  sensors. By combination of several textile pressure sensors, the sensor array is able to measure the pressure on a single-point region, as well as the distributions.

**C. Pressure Points And Placement**

The pressure sensing area of the foot can be divided into 15 areas, as heel (area 1–3), midfoot (area 4–5), metatarsal (area 6–10), and toe (area 11–15), as shown in Fig. 2. These areas support most of the body weight and adjust the body balance. The measured force at these positions can be used to derive physiological, function information of the

lower limbs and whole body. In order to reduce the system complexity, eight positions as indicated in fig 3 were selected at heel and metatarsal areas in the first prototype shoe, because these areas have higher pressure during normal activities of children, young, and old adults. Exact locations of sensors can be determined by depth shape of the subject’s foot in soft model. Earlier methods considered utilizing five sensors at the positions of heel, metatarsal, and hallux to achieve a clinical gait analysis. Another system was presented for a gait-phase detection system using three sensors at underneath the heel and metatarsal areas. Six sensors at the heel and metatarsal positions are adequate for such clinical investigation in gait analysis. For sports and fitness, the Nike +iPod Sport Kit used just one sensor in the midfoot to measure the wearer’s pace, distance, and energy consumption during running.

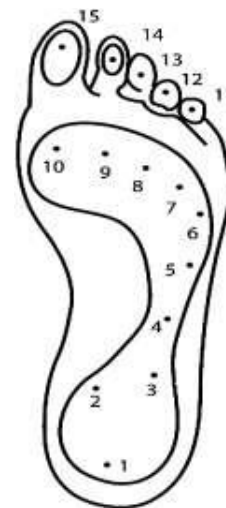


Fig. 2. Various Pressure sensing Points

The Adidas-1 running shoe uses one sensor at the heel position to provide compression measurement for adjusting to running situation. Hence, six sensors are sufficient for sport or fitness assessments. Ideally, adding additional sensors at hallux and midfoot positions will enlarge the application scopes. As the textile sensor is relatively cheap and has a good fatigue resistance, it is easy to add more sensors in other applications.



Fig. 3. Placement of sensors



In order to reduce the system complexity, eight positions (see Fig. 3) can be selected, because these areas have higher pressure during normal activities. A connector is attached to the sensors to transfer data to the circuit. Through the connector, voltage signals on the sensors are extracted and then sent to the embedded analog-to-digital (A/D) converter channels in the processor. Finally, these values are wirelessly transmitted to a remote receiver by an antenna. The data acquisition system has the following advantages.

- 1) Small size and light weight.
- 2) Large transmission range.
- 3) Stable and repeatable performance.
- 4) Rechargeable battery configuration.

#### D. Circuit Design

Fig 4 illustrates the typical implementation requirements. The selected position of sensors are wired to signal conditioning and amplification IC. A processor capable of handling eight channels of analog values and which can provide sufficient conversion accuracy is selected. An ARM based LPC2148 has been selected for this purpose. After processing the data it is given to the serial port and then to the wireless transmitter.

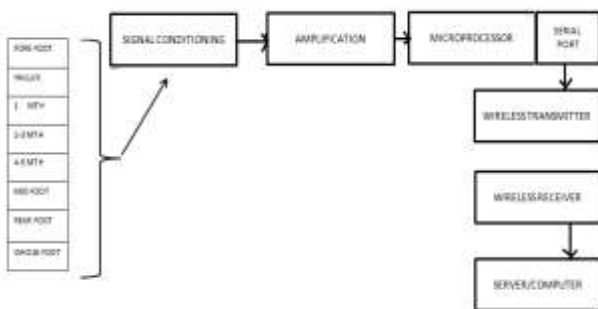


Fig 4. Design Essentials

#### E. Wireless Architecture

Several radio protocols and open standards are now available, however, most of them do not support multiple sensors and are not compatible with low-power radio hardware. For this reason, we chose IEEE 802.15.4, which in recent years has emerged as the dominant wireless protocol for low-power sensor networks, and is also the physical-layer protocol for Zigbee. A wireless platform using Ultra Wide Band standard IEEE 802.15.4a is a possible alternative in the future. Using a star topology for our network will minimize processing overhead and power consumption.

The data acquisition system is designed with small size and stable to power supply interference. There are three possible ways to interpret the acquired data. Bluetooth virtual serial port technology can be utilized to interface the circuit to mobile and PDAs. A Zigbee receiver and a laptop environment can increase the coverage area of the system so that the subject can be

tested outdoor. Another possible alternative is to transfer the data to a remote web server, so that remote monitoring and data collection is possible. These configurations make the system suitable for research laboratories, clinics, and daily outdoor/indoor activities.

#### F. Processor Module

The LPC2148 microcontrollers are based on a 32/16 bit ARM7TDMI-S CPU with embedded high speed flash memory ranging from 32 kB to 512 kB. A 128-bit wide memory interface and a unique accelerator architecture enable 32-bit code execution at the maximum clock rate. For critical code size applications, the alternative 16-bit Thumb mode reduces code by more than 30 % with minimal performance penalty. Due to their tiny size and low power consumption, LPC2148 is ideal for applications where miniaturization is a key requirement. A blend of serial communications interfaces ranging from a USB 2.0 Full Speed device, multiple UARTS and on-chip SRAM of 8 kB upto 40 kB, make these devices very well suited for communication gateways. Dual 10-bit ADC(s) with conversion times as low as 2.44 microseconds per channel make these microcontrollers particularly suitable for industrial control and medical systems. CPU operating voltage range of 3.0 V to 3.6 V makes it operable with batteries.

#### G. Radio Module

The radio module uses a Chipcon CC2420. The reference voltage on these inputs can be configured via wireless commands from the radio base station. The IEEE802.15.4 protocol can be implemented in firmware with independent sampling and transmission intervals that can be set via wireless commands from the base station. Every transmission cycle, the radio module wakes up, and then, in turn activates the power enable in on the sensor module to power up the sensors. After a 10 ms delay, the radio module captures a 10-bit A/D sample from each of the sensors, transmits the data packet to the base station, and then goes back to sleep.

#### H. Transmission Power And Operating Range

The CC2420 radio IC has a maximum transmission power of 1 mW (0 dBm), which provides a wireless detection range of 50–75 m in free space using a 5 dBi gain receiver antenna.

Indoor range is significantly less and depends on the building layout, but is approximately 15–20 m for the module with integrated antenna and 8–10m for the version with external antenna. These wireless operating distances are sufficient for our current health and medical research needs.



I. Radio Base Station

A popular method that is used to collect data from multiple radio modules and sensors is universal serial bus (USB), which has a USB interface to plug into PC's and laptops. For software development a platform of OS which is easier to use has been adopted. Accordingly Windows is the platform used to develop the front end. Fig 5 shows the means by which an environment for software development has been utilized. The software is designed in such a manner that it is capable of providing secured entry to use the software using authentication. It is also possible to set the various sensing points that are to be added for data collection. Also provision had been made to set the serial data rates and other parameter by front end module. The hardware setup placed inside the sole wirelessly transmits the pressure values to the receiving module connected to the serial port. This information is store in a database continuously. Further processing is done by the front end software.

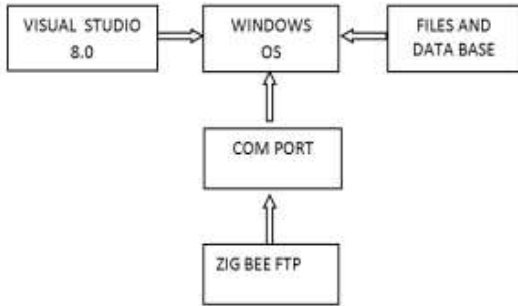


FIG 5. Software development.

Upon start up various configurations are made. These settings are transferred through serial port to the wireless module. This in turn sends these setting to the remote hardware. Upon successful configuration the start data collection process is initiated. Wherein the data from the hardware is received wirelessly. These data are stored in a buffer after which the system waits for the next data to arrive. This sequence is repeated until a stop signal is given from the software.

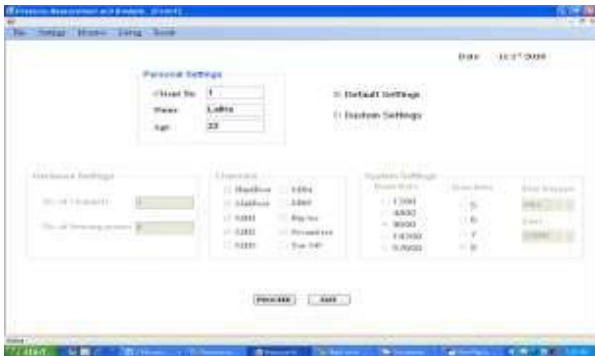


FIG 6. Configuration By Software

Fig 6 shows the actual settings window where personal details sensor point settings and other system settings are done in software to configure hardware.

The data thus received is used for various calculations.

$$\text{Mean} = \text{Sum} (P1, \dots Pi, \dots Pn) / n$$

$$\text{Peak} = \text{Max}(P1, \dots Pi, \dots Pn)$$

IV. RESULTS

Results have been plotted as real time graphical displays and the peak and mean pressure are also displayed. A pie chart showing the distribution of pressure has also been given. Fig 7 shows pressure distribution at various sensing points. This gives an idea about where the maximum pressure that was recorded during the entire record time. A real time signal display window shows the values as recording is done which helps in monitoring instantaneous real time pressure values.



FIG 7. Pressure Distribution Display

Fig 8 shows a sample recorded output recording from software as signal variations. We can start, stop recording and store the recorded values to be viewed later for analysis.

FIG 8. Real Time Display



V. CONCLUSION AND FUTURE WORK

As demonstrated in this paper, recent advances in low-power radio electronics and wireless protocols are enabling the development of new technology for long-term, comfortable sensing of pressure information in new areas of health and medical research. New wearable materials, coupled with small long lasting batteries, now provide the means to collect data over much longer time scales and in nonclinical settings, and the means for



individuals to control the collection and communication of data by easily putting on or taking off the sensor (not needing the help of a researcher, and not having data sensed from them if they do not want to be sensed). It has been shown data and evaluations in this paper to indicate that these new sensors, while non traditional in their placement and design, are capable of gathering data comparable to data gathered with traditional sophisticated sensors. Thus, the system we have developed provides an important contribution over existing systems for gathering data in long-term naturalistic settings. It is our goal to help make lightweight portable sensor platforms such as the ones presented here accessible to a wider number of researchers and to individuals who wish to have help understanding and communicating their foot pressure changes. We envision that the strong connection between affective computing and health will also lead to new forms of understanding, diagnosing, and supporting the growing number of people interested in footwear evaluation, athletic training, clinical gait analysis, and pathology foot diagnosis. Research on the area of developing a stand alone hand held device to the entire monitor the above method would be considerable development. Also the scope to transfer the recorded data through internet for data analysis to experts in any location and give feedback.

## REFERENCES

- [1] L. A. Lavery, S. A. Vela, J. G. Fleishli, D. G. Armstrong, and D. C. Lavery, - Reducing plantar pressure in the neuropathic foot—A comparison of footwear, *Diabetes Care*, vol. 20, no. 11, pp. 1706–1710, 1997.
- [2] S. J. Morris and J. A. Paradiso, -Shoe-integrated sensor system for wireless gait analysis and real-time feedback, *Proc. 24th Annu. Conf. Annu. Fall Meet. Biomed. Eng. Soc. EMBS/BMES Conf.*, Houston, 2002, pp. 2468–2469. [3] Q. , H. Wei, W. , L. Lu, Z.Y. Fu, and S. B. Lu, -A new system for foot pressure measurement and gait analysis, *Chin. J. Biomed. Eng.*, vol. 19, no. 1, pp. 32–40, 2000.
- [4] E. Kellis, -Plantar pressure distribution during barefoot standing, walking and landing in preschool boys, *Gait Posture*, vol. 14, no. 2, pp. 92–97, 2001. [5] M. , J. Hessert, M. Vyas, J. Leach, K. Hu, L. , A. Lipsitz, and V. Novak, -Foot pressure distribution during walking in young and old adults, *BMC Geriatr.*, vol. 5, p. 8, 2005.
- [6] S. Bamberg, A. Y. Benbasat, D. M. Scarborough, D. E. Krebs, and J. A. Paradiso, -Gait analysis using a shoe-integrated wireless sensor system, *IEEE Trans. Inf. Technol. Biomed.*, vol. 12, no. 4, pp. 413–423, Jul. 2008.